

 CLEARFIX



CLEARFIX RIGID STERNAL FIXATION

 CLEARFLOW
Distribution Company

CLEARFIXSYSTEM.COM




Surgical Technique	04
Ordering Information: Plates	06
Ordering Information: Screws	07
Ordering Information: Instruments	08
ClearFix Rigid Sternal Fixation Set Configuration	12



INDICATIONS

The ClearFix Rigid Sternal Fixation is intended for use in the stabilization and fixation of fractures of the anterior chest wall including sternal fixation following sternotomy and sternal reconstructive surgical procedures to promote fusion.

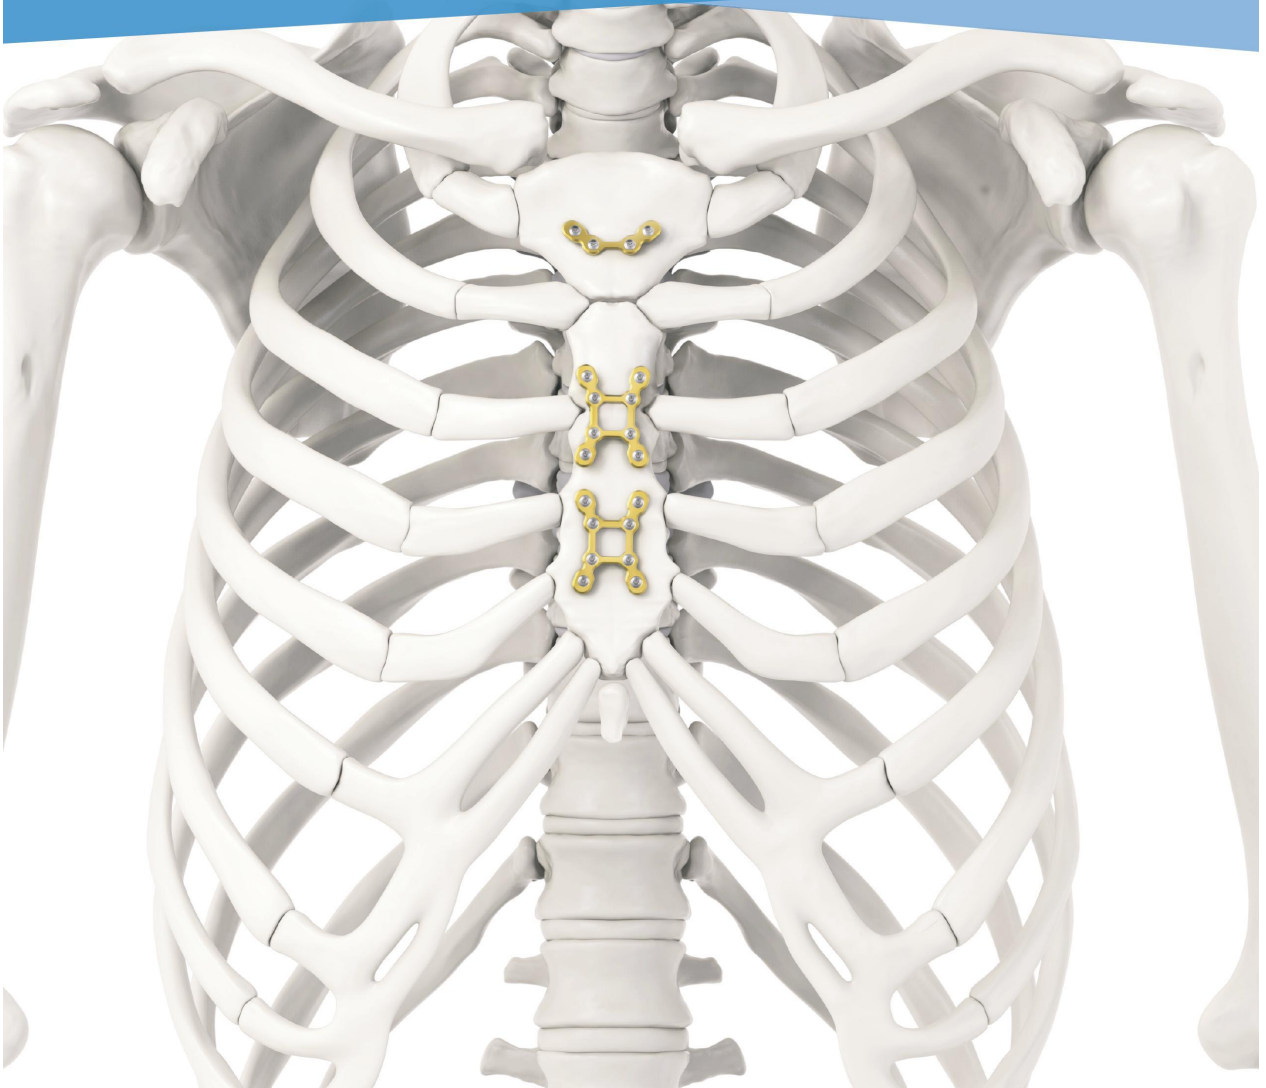


SURGICAL TECHNIQUE

1 Measuring Sternal Depth


Measure sternal depth where plate placement will occur. Measure at 3 points (manubrium, body and xiphoid). In the photo, the measuring device indicates that a 14 mm screw length would be recommended for plate placement. The measuring device accounts for the thickness of the plate, so a 14 mm screw would be used in this example.

*Note, if using a standard ruler to measure the thickness of the sternum, you should use the next highest even numbered length screw to account for the plate thickness. For example a sternal thickness of 8 mm - 9 mm should utilize a 10 mm screw, while a sternal thickness of 10 mm - 11 mm should use a 12 mm screw. Surgeons should always determine screw size based on the patient's anatomy.

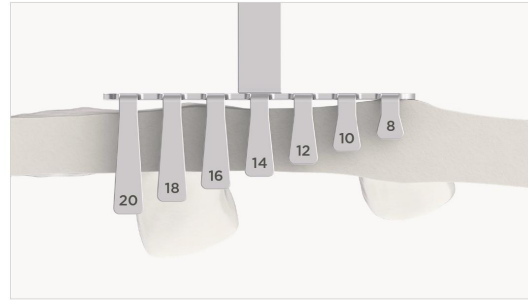


2 Bone Reduction and Plate Positioning

Wire the manubrium and xiphoid to reduce the top and bottom of the sternum. Complete the full approximation by placing reduction forceps at the mid-body.

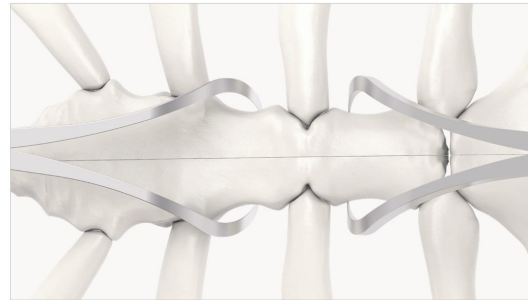


Required Set

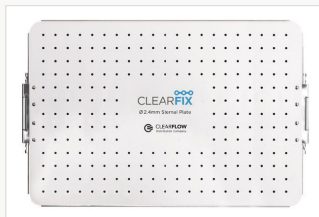

ClearFix Rigid Sternal Fixation Kit
CF-112-107

Required Instruments



Depth Gauge (Mid)
CF-111-148



Bone Reposition Forcep (Large)
CF-111-154




Bone Reposition Forcep
CF-111-155

3 Fixation of the Plate

Plates are two-sided to facilitate placement. If necessary, bend the plate to match the shape of the bone.

Insert screws into the plate. Using the Power Driver for screw insertion is recommended for quick and efficient surgery.

Fully tighten once additional screws are in place by using the screw driver handle.

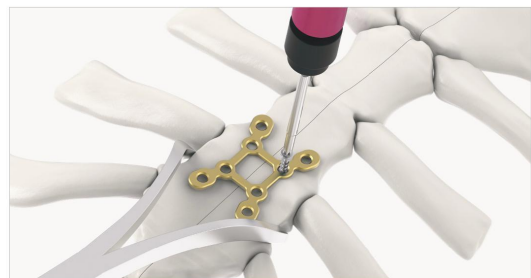

Required Instruments



Plate Bender
CF-26.0240.17




Plate Cutter
CF-111-156



**Torque 40Ncm,
165 RPM**
CF-111-ED-051



Screw Driver Handle
CF-111-151

ORDERING INFORMATION: PLATES

CLEARFIX RIGID STERNAL FIXATION



CF-24-LPST-004

L
4 Holes
1.6 mm
Gold



CF-24-XPST-008

X
8 Holes
1.6 mm
Gold




CF-24-SQST-004

Square
4 Holes
1.6 mm
Gold




CF-24-JLST-008

JL
8 Holes
1.6 mm
Gold

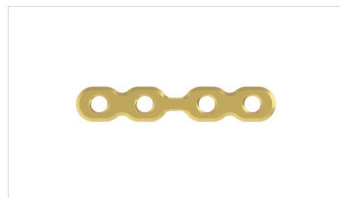

CF-24-STST-004

Straight
4 Holes
1.6 mm
Gold

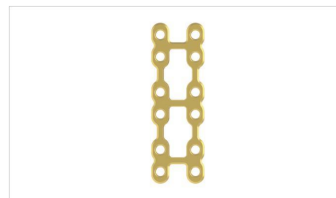

CF-24-HNST-012

Ladder, Narrow
12 Holes
1.6 mm
Gold



CF-24-STST-008

Straight
8 Holes
1.6 mm
Gold



CF-24-HWST-012

Ladder, Wide
12 Holes
1.6 mm
Gold



CF-24-HSST-008

Ladder, Short
8 Holes
1.6 mm
Gold



ORDERING INFORMATION: SCREWS

CLEARFIX RIGID STERNAL FIXATION

Ø 2.4 LOCKING SCREWS

	Code	Length	Color	Set Quantity
	CF-24L-SA-S08-TA	8 mm	Silver	7
	CF-24L-SA-S10-TA	10 mm	Silver	14
	CF-24L-SA-S12-TA	12 mm	Silver	14
	CF-24L-SA-S14-TA	14 mm	Silver	14
	CF-24L-SA-S16-TA	16 mm	Silver	14
	CF-24L-SA-S18-TA	18 mm	Silver	7

Ø 2.7 LOCKING SCREWS

	Code	Length	Color	Set Quantity
	CF-27L-SA-S08-TA	8 mm	Gold	4
	CF-27L-SA-S10-TA	10 mm	Gold	8
	CF-27L-SA-S12-TA	12 mm	Gold	8
	CF-27L-SA-S14-TA	14 mm	Gold	8
	CF-27L-SA-S16-TA	16 mm	Gold	8
	CF-27L-SA-S18-TA	18 mm	Gold	4

INSTRUMENTS

CLEARFIX RIGID STERNAL FIXATION

HANDLE



Code	Description	Set Quantity
CF-111-151	Screw Driver Handle	1

PLATE BENDER



Code	Description	Set Quantity
CF-26.0240.17	Plate Bender	2

PLATE CUTTER



Code	Description	Set Quantity
CF-111-156	Plate Cutter	1



BONE REPOSITION FORCEP



Code	Description	Set Quantity
CF-111-154	Bone Reposition Forcep (Large)	2
CF-111-155	Bone Reposition Forcep	2

DEPTH GAUGE



Code	Description	Set Quantity
CF-111-148	Depth Gauge (Mid)	1
CF-111-149	Depth Gauge (Left)	Optional
CF-111-150	Depth Gauge (Right)	Optional

ORDERING INFORMATION: INSTRUMENTS

CLEARFIX RIGID STERNAL FIXATION

DRIVER



Code	Description	Set Quantity
CF-113-HF-613	Driver for T8 Φ3 Standard 70mm Ball	1
CF-113-HF-624	Driver for T8 Φ3 Standard 50mm Ball	1


FORCEPS



Code	Description	Set Quantity
CF-111-038	Plate Holding Forcep	1
CF-114-009	Plate Holding Forcep	1



POWER DRIVER

		
Code	Description	Set Quantity
CF-111-ED-050	Torque 45Ncm, 210 RPM	Optional
CF-111-ED-051	Torque 40Ncm, 165 RPM	Optional

KIT

		
Code	Description	Set Quantity
CF-112-107	ClearFix Rigid Sternal Fixation Kit (Includes Inner Tray)	1

CLEARFIX RIGID STERNAL FIXATION SET CONFIGURATION

PLATES (NON-STERILE)

No.	Code	Description	Set Quantity
1	CF-24-LPST-004	L Plate, 4 Holes, T=1.6mm, Bridge=2.4mm, Gold	3
2	CF-24-SGST-004	Square Plate, 4 Holes, T=1.6mm, Bridge=2.4mm, Gold	3
3	CF-24-HSST-008	Ladder Plate, Short, 8 Holes, T=1.6mm, Bridge=2.4mm, Gold	3
4	CF-24-STST-004	Straight Plate, 4 Holes, T=1.6mm, Bridge=2.4mm, Gold	3
5	CF-24-STST-008	Straight Plate, 8 Holes, T=1.6mm, Bridge=2.4mm, Gold	3
6	CF-24-XPST-008	X-Plate, 8 Holes, T=1.6mm, Bridge=2.4mm, Gold	3
7	CF-24-JLST-008	JL Plate, 8 Holes, T=1.6mm, Bridge=2.4mm, Gold	3
8	CF-24-HWST-012	Ladder Plate, Wide, 12 Holes, T=1.6mm, Bridge=2.4mm, Gold	3
9	CF-24-HNST-012	Ladder Plate, Narrow, 12 Holes, T=1.6mm, Bridge=2.4mm, Gold	3

SCREWS (NON-STERILE)

No.	Code	Description	Set Quantity
1	CF-24L-SA-S08-TA	Ø2.4 Screw, 8mm, Self-Drilling, Cancellous, Locking, Starix	7
2	CF-24L-SA-S10-TA	Ø2.4 Screw, 10mm, Self-Drilling, Cancellous, Locking, Starix	14
3	CF-24L-SA-S12-TA	Ø2.4 Screw, 12mm, Self-Drilling, Cancellous, Locking, Starix	14
4	CF-24L-SA-S14-TA	Ø2.4 Screw, 14mm, Self-Drilling, Cancellous, Locking, Starix	14
5	CF-24L-SA-S16-TA	Ø2.4 Screw, 16mm, Self-Drilling, Cancellous, Locking, Starix	14
6	CF-24L-SA-S18-TA	Ø2.4 Screw, 18mm, Self-Drilling, Cancellous, Locking, Starix	7
7	CF-27L-SA-S08-TA	Ø2.7 Emergency Screw, 8mm, Cancellous, Locking, Starix	4
8	CF-27L-SA-S10-TA	Ø2.7 Emergency Screw, 10mm, Cancellous, Locking, Starix	8
9	CF-27L-SA-S12-TA	Ø2.7 Emergency Screw, 12mm, Cancellous, Locking, Starix	8
10	CF-27L-SA-S14-TA	Ø2.7 Emergency Screw, 14mm, Cancellous, Locking, Starix	8
11	CF-27L-SA-S16-TA	Ø2.7 Emergency Screw, 16mm, Cancellous, Locking, Starix	8
12	CF-27L-SA-S18-TA	Ø2.7 Emergency Screw, 18mm, Cancellous, Locking, Starix	4



INSTRUMENTS


No.	Code	Description	Set Quantity
1	CF-111-ED-050	Torque 45Ncm, 210 RPM	Optional
2	CF-111-ED-051	Torque 40Ncm, 165 RPM	Optional
3	CF-111-038	Plate Holding Forcep	1
4	CF-111-154	Bone Reposition Forcep (Large)	2
5	CF-111-155	Bone Reposition Forcep	2
6	CF-111-156	Plate Cutter	1
7	CF-26.0240.17	Plate Bender	2
8	CF-111-148	Depth Gauge (Mid)	1
9	CF-113-HF-613	Driver for T8 Φ 3 Standard 70mm Ball	1
10	CF-113-HF-624	Driver for T8 Φ 3 Standard 50mm Ball	1
11	CF-114-009	Plate Holding Forcep	1
12	CF-111-151	Screw Driver Handle	1
13	CF-112-107	ClearFix Rigid Sternal Fixation Kit (Includes Inner Tray)	1
14	CF-111-149	Depth Gauge (Left)	Optional
15	CF-111-150	Depth Gauge (Right)	Optional

ABOUT CLEARFLOW DISTRIBUTION COMPANY

ClearFlow Distribution Company helps cardiac surgery professionals improve outcomes and advance healing through sustainable medical technologies that protect a patient's quality of life.

We believe that there is nothing more beautiful than getting patients back home to their lives and their loved ones faster.



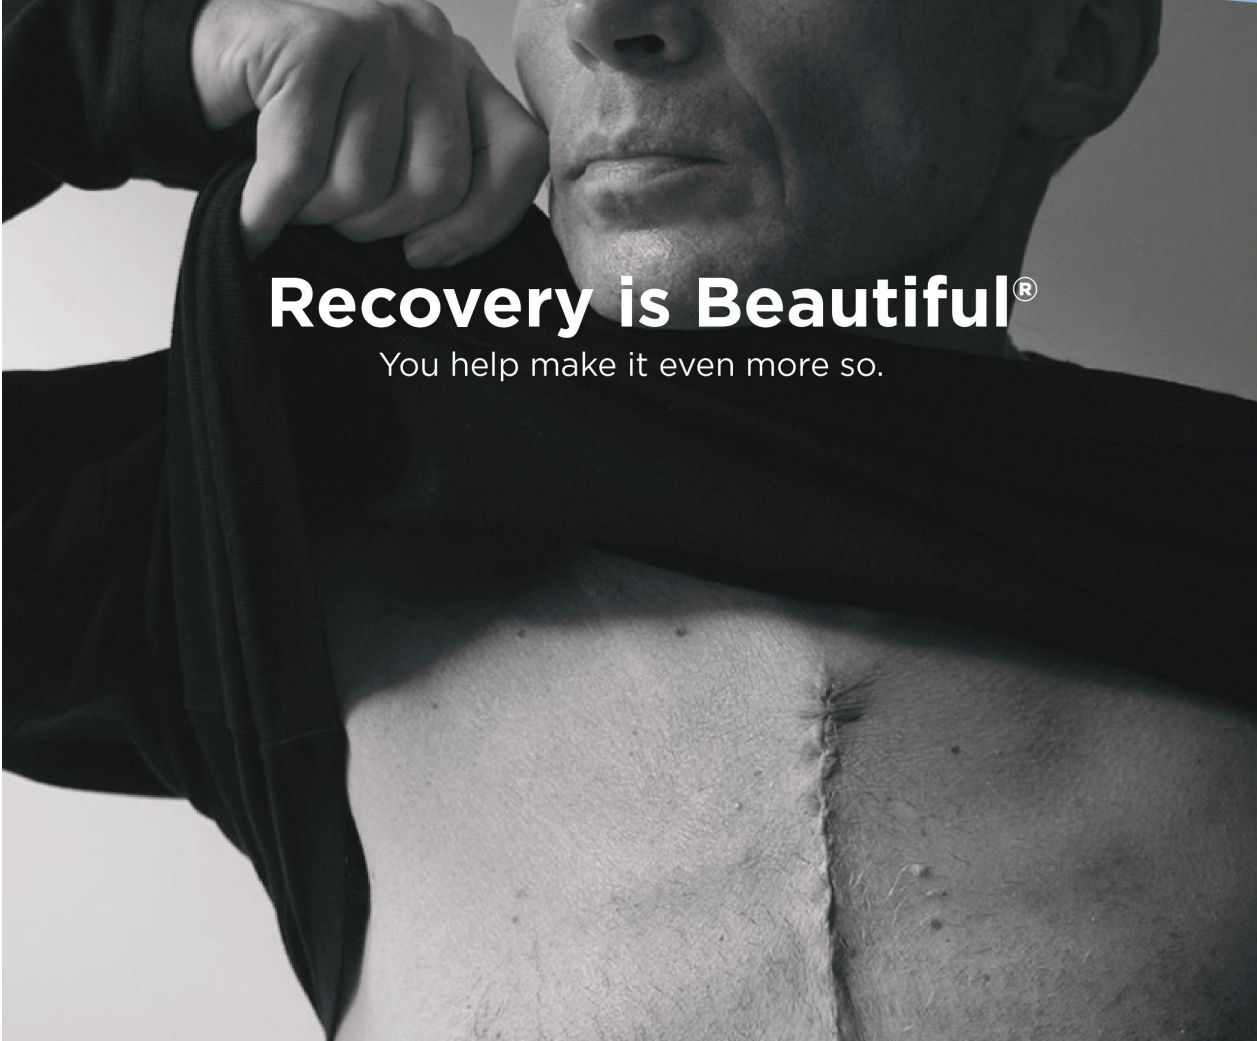

Recovery is Beautiful[®]

You help make it even more so.


CLEARFIX



 **CLEARFLOW**
Distribution Company

CLEARFIXSYSTEM.COM